



Megazyme,
Bray Business Park,
Bray, Co. Wicklow,
A98 YV29,
Ireland.
Tel: + 353 1 286 1220
Fax: + 353 1 286 1264

Validation Report: D-Glucose HK Assay Kit (cat. no. K-GLUHK)

1. Scope

Megazyme's D-Glucose HK Assay Kit (K-GLUHK) is an enzymatic method used for the rapid measurement and analysis of D-glucose in foodstuffs, plants and other materials. This method was developed in-house and measures glucose in g/L. Methods based on this principle have been accepted by AOAC, EN, NEN, NF, DIN, GOST, OIV, IFU, AIJN and MEBAK.

2. Planning

The purpose of this report is to verify and validate the current method as detailed by D-Glucose HK Assay Kit (K-GLUHK).

3. Performance characteristics

The selectivity, working range, limit of detection, limit of quantification, trueness (*bias*) and precision of this kit is detailed in this report.

3.1. Selectivity

This assay is specific for D-glucose.

Interfering substances in the sample being analysed can be identified by including an internal standard. Quantitative recovery of this standard would be expected. Losses in sample handling and extraction are identified by performing recovery experiments, i.e. by adding D-glucose to the sample in the initial extraction steps.

3.2. Working Range


Assay follows the D-Glucose HK Assay Kit (K-GLUHK) standard procedure. 0.1 mL of D-glucose standard was used as sample, with a range of concentrations (0.04-0.8 g/L D-glucose) which corresponds to 4-80 µg of D-glucose per cuvette. Absorbance A₂ was read after 5 min, at 340 nm and at 25°C as recommended in the procedure.



Megazyme,

Bray Business Park,
Bray, Co. Wicklow,
A98 YV29,
Ireland.
Tel: + 353 1 286 1220
Fax: + 353 1 286 1264

D-Glucose Concentration [$\mu\text{g}/\text{assay}$]	$\Delta A_{340\text{nm}}$
0	0.000
4	0.063
8	0.122
20	0.305
30	0.451
40	0.602
60	0.908
80	1.203

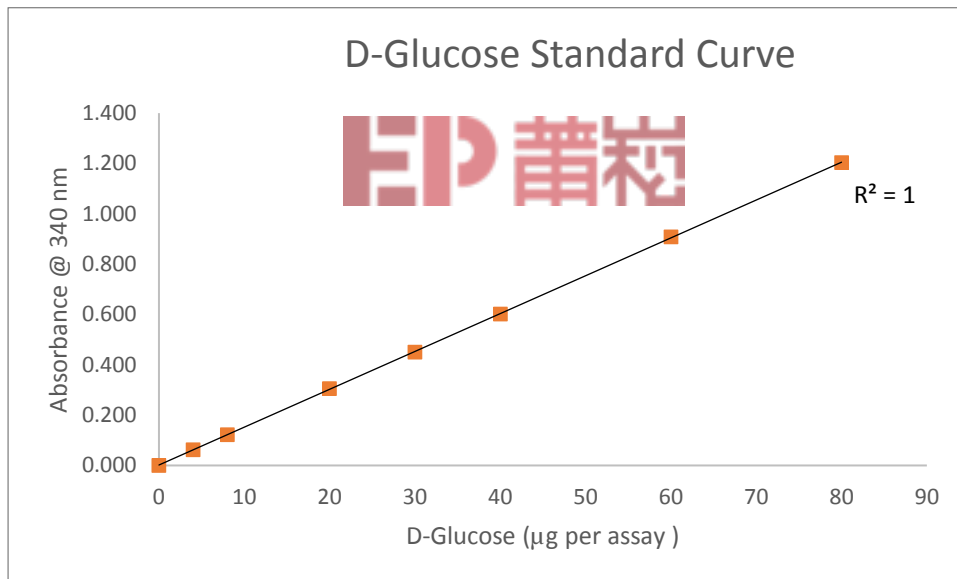



Megazyme,

Bray Business Park,
Bray, Co. Wicklow,
A98 YV29,
Ireland.
Tel: + 353 1 286 1220
Fax: + 353 1 286 1264

3.3. LOD and LOQ

The **instrument limit of detection**, as per kit booklet, is 0.663 mg/L, which is derived from an absorbance difference of 0.020 with the maximum sample volume of 2.00 mL.

The **calculated limit of detection (LOD)** and the **calculated limit of quantification (LOQ)** for this report purpose is based on the analysis of samples that have been taken through the whole D-Glucose HK Assay Kit (K-GLUHK) measurement procedure.

- The LOD is the lowest concentration of the analyte that can be detected by the method. LOD is calculated as $3 \times s'0$; where $s'0$ is the standard deviation of a number of samples A1 reading.
- The LOQ is the lowest level at which the kit's performance is acceptably repeatable. LOQ is calculated as $kQ \times s'0$; where $s'0$ is the standard deviation of a number of samples A1 reading. The IUPAC default value for kQ is 10
- For D-Glucose HK Assay Kit (K-GLUHK)

LOD – For 2.0 mL of sample (maximum volume)

D-Glucose = 0.050 mg/L

LOQ – For 2.0 mL of sample (maximum volume)

D-Glucose = 0.150 mg/L

* **Note:** The above detection limits are for samples as used in the assay, after sample preparations if required (e.g. deproteinisation). The dilution used in pre-treatment must be accounted for while establishing the detection limits for specific samples.



Megazyme,

Bray Business Park,
 Bray, Co. Wicklow,
 A98 YV29,
 Ireland.
 Tel: + 353 1 286 1220
 Fax: + 353 1 286 1264

3.4. Trueness (*Bias*)

Comparison of the mean of the results (x) achieved with D-Glucose HK Assay Kit (K-GLUHK) method with a suitable reference value (x ref). For this report, Relative Bias is calculated in per cent as: $b(\%) = \frac{x - x_{ref}}{x_{ref}} \times 100$. The reference material for this purpose is D-glucose supplied with the D-Glucose HK Assay Kit (K-GLUHK) at 0.4 g/L

Relative Bias *b*(%)

	n	Ref Material (g/L)	Mean (g/L)	<i>b</i> (%)
D-Glucose	20	0.4	0.4016	0.58

3.5. Precision

This report details the reproducibility of the D-Glucose HK Assay Kit (K-GLUHK), it is a measure of the variability in results, on different days and by different analysts, over an extended period of time.

For the purpose of this report different lot numbers of the kit standard is used as the reference material.

Reproducibility

	n	Ref Material (g/L)	Mean (g/L)	Standard Deviation	%CV
D-Glucose	20	0.4	0.4016	0.0070	1.73

Repeatability of this kit can be assessed using wine samples. This is a measure of the variability in results by a single analyst, using real samples, using the same equipment and over a short period of time. The use of wine samples shows one of the many applications of this kit.

Repeatability

Glucose	n	Mean (g/L)	Standard Deviation	%CV
White Wine	6	1.396	0.025	1.79
Red Wine	6	0.4	0.007	1.75



Megazyme,

Bray Business Park,
Bray, Co. Wicklow,
A98 YV29,
Ireland.
Tel: + 353 1 286 1220
Fax: + 353 1 286 1264

4. Conclusion

The method outlined in this document is a robust, quick and easy method for the measurement of D-glucose in various matrices. It has been used for many years and is fully automatable for high throughput analysis of samples. Data presented in this report verifies and validates that this method is fit for the purpose intended, which is summarised below.

Validation Summary	Glucose
Working range (μg in cuvette)	4-80
LOD (mg/L)	0.05
LOQ (mg/L)	0.15
Relative Bias <i>b</i> (%)	0.58
Reproducibility (%CV using kit standard)	1.73
Repeatability (%CV using white wine)	1.79
Repeatability (%CV using red wine)	1.75

EP 葡粒